

Port 031 – Infrared

This beamline is SRC owned.

Current as of June 2012


Beamline

Infrared Spectromicroscopy
608-877-2031

Manager

Mark Bissen
608-877-2146

mbissen@src.wisc.edu

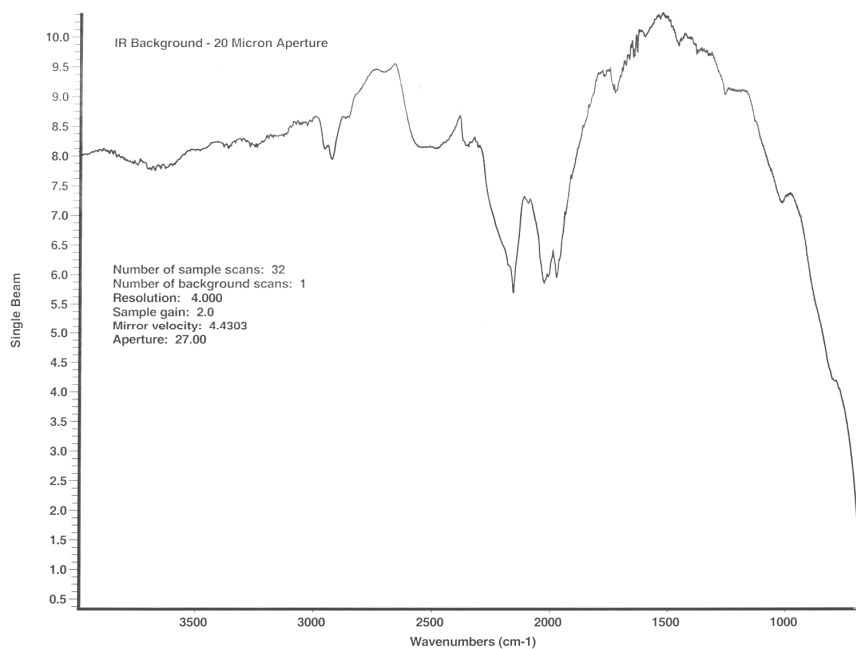

Technical

Energy Range	650 – 8000 cm ⁻¹
Minimum Bandpass	0.125 cm ⁻¹
Focused Spot	Collimated output light beam; position is 965 mm above floor. Spot size (horizontal x vertical) is 25 mm x 12 mm.
Automation	Computer controlled scanning
Special Feature(s)	Infrared microscope with programmable mapping stage